



Füllstand



Druck



Durchfluss



Temperatur

Flüssigkeits-  
analyse

Registrierung

Systeme  
Komponenten

Services



Solutions

## Technical Information

# Mycom S CLM153

One or two circuit transmitter for conductive or inductive conductivity, with controller and limit value functions, for Ex or non-Ex areas



### Application

The four-wire transmitter Mycom S CLM153 is optimally suited for conductivity measurement and resistivity measurement in the following areas of process engineering and processing systems:

- Chemical processes
- Food technology
- Pharmaceuticals
- Water treatment
- Explosion hazardous areas



### Your benefits


- High measurement reliability:
  - Monitoring of the measuring signal
  - Polarisation monitoring
  - Numerous temperature compensation methods including neutral and acid ultra pure water compensation
  - Logbook functions and data log
  - Redundancy and differential measurement
- High user friendliness:
  - Integrated cleaning function Chemoclean
  - Online help
- Individually adaptable:
  - Optional two-circuit measurement (galvanically isolated)
  - Extended controller and limit value functions
  - Current and resistance inputs for feedforward control and position feedback
  - Plug-in module to save and transfer configuration (DAT)
  - Output contacts according to NAMUR
  - Limit value function acc. to USP (US Pharmacopeia)
  - pH value from the differential conductivity acc. to VGB (Vereinigung der Großkraftwerksbetreiber e.V. / Ass. of power and heat generating utilities)
- Ex approval: ATEX II (1) 2 G EEx em [ia/ib] IIC T4
- HART or PROFIBUS PA (Profile 3.0) certified

## Function and system design

### Measuring system

A complete measuring system comprises:

- Transmitter Mycom S CLM153
- Conductivity sensor with integrated temperature sensor Pt100:
  - conductive, e.g. CLS12, CLS13, CLS14, CLS15, CLS16, CLS21 oder
  - inductive, e.g. CLS50, CLS52
- Welded socket or assembly for pipe or tank installation
- Conductivity measuring cable, e.g. CPK9 (with TOP68 plug for CLS16), CLK5 (inductive), CLK71 (conductive)

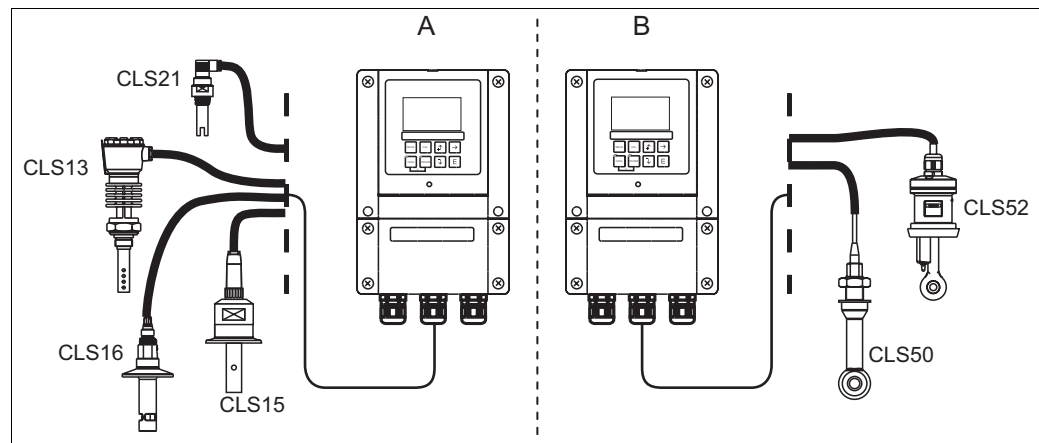

00 7-CLM153rev-1 4-08-00-wr-001.EPS

Measuring system

- A     Conductive conductivity measurement  
 B     Inductive conductivity measurement

### Important functions

#### Polarisation detection

Polarisation effects in the boundary layer between the sensor and the solution to be measured limit the measuring range of conductive conductivity sensors.

The CLM 153 transmitter can detect polarisation effects using an innovative, intelligent signal evaluation process.

#### Process Check System (PCS)

This function checks the measuring signal for deviations. If the measuring signal does not change for some time (several measured values), an alarm is triggered. Soiling, blockage or similar could be the cause of such behaviour.

#### Logbooks

There are several logbooks available. The last 30 entries are saved to an error log, an operation log and a calibration log. The entries are displayed with their date and time.

#### Parameter set switching (PSS)

Inductive measuring systems in particular are equipped with measuring range switching devices because of the large spans they cover.

The CLM 153 transmitter provides the benefit of parameter set switching, remote controlled via binary inputs:

- current output ranges
- operation mode (e.g. conductivity or concentration measurement)
- temperature compensation
- limit values

### Two-circuit: differential measurement

A two-circuit device allows you to connect two sensors of the same type to measure and monitor differential conductivity.

This is necessary for:

- Media separation
- Monitoring heat exchangers
- Monitoring ion exchangers
- Determination of the pH value acc. to the VGB-R 450L rule for boiler feed water in power plants.

Conditions are:

- Basic operation of the boiler feed water circuit (conditioning with NaOH or  $\text{NH}_3$ )
- Impurities consist of NaCl only (practically no phosphates (<0.5 mg/l))
- For pH<8 the impurity concentration must be low in relation to the alkalisation agent.

### Two-circuit: efficiency

The two-circuit device allows you to display the two measured values ("A" and "B") according to their efficiency.

You can select from the following:

- A – B
- B – A
- A/B
- B/A
- (A – B)/A
- (B – A)/A
- (A – B)/B
- (B – A)/B

in the following units: auto,  $\mu\text{S}/\text{cm}$ ,  $\text{mS}/\text{cm}$ ,  $\text{S}/\text{cm}$ ,  $\mu\text{S}/\text{m}$ ,  $\text{mS}/\text{m}$ ,  $\text{S}/\text{m}$  bzw. auto,  $\text{k}\Omega\text{cm}$ ,  $\text{M}\Omega\text{cm}$ ,  $\text{k}\Omega\text{m}$ , % and without unit (quotient).

### United States Pharmacopeia (USP)


The requirements on ultrapure water in the pharmaceutical industry are specified by the American USP.

Mycom S CLM 153 meets the USP requirements on conductivity measuring systems:

- Precise temperature measurement at point of conductivity measurement
- Simultaneous display of uncompensated conductivity values and temperature
- Display resolution 0.001  $\mu\text{S}/\text{cm}$
- Exact adjustment of the transmitter in the factory with traceable precision resistances
- Exact adjustment of the sensors in the factory in accordance with ASTM D 1125-9 resp. ASTM D 391-99
- Temperature-dependent measurement value monitoring in accordance with USP.

### Data log

You can record two freely selectable parameters using the integrated data logs and then display the results graphically in real time. You can retrieve the 500 most recently measured values using date and time. In this way, you can graphically display the process flow. This is a quick way of checking the process and provides a good opportunity for optimising conductivity control.

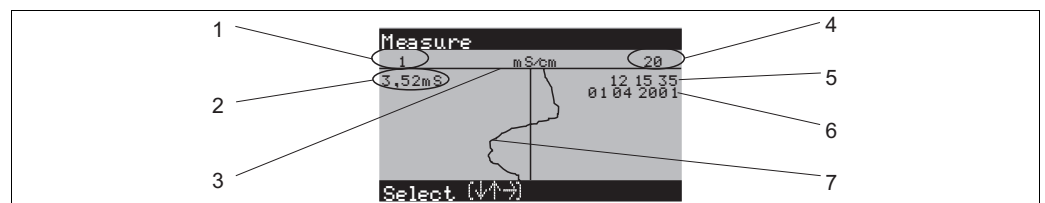

C07-CLM153a-20-06-00-en-100.eps

Example of data log 1

- |   |  |
|---|--|
| 1 Minimum display range (selectable to 0 $\mu\text{S}/\text{cm}$ )  | 5 Time when this measured value was recorded |
| 2 Measured value of the current scroll bar position                 | 6 Date when this measured value was recorded |
| 3 Scroll bar  | 7 Measured value graph                       |
| 4 Maximum display range (selectable to 2000 $\text{mS}/\text{cm}$ ) |  |

### Cleaning functions

The Chemoclean® spray cleaning system automatically cleans the electrode. It is controlled by two contacts (possible with basic version). Cleaning can be triggered automatically at programmed intervals, manually or by an error message. You can configure almost any error to trigger cleaning.

### Simple control

The following control functions are integrated in Mycom:

- Limit value contact: two-point controller with hysteresis for simple temperature control for example
- PID controller:
  - For one and two-sided processes
  - With freely adjustable P, I and D components
  - Including configurable range-dependent gain (segmented curve)
  - Differentiation between batch and online processes
- Manipulated variable output
  - The manipulated variable can be output either as binary signal via the relays or via the current output:
  - Binary signal via relays as PWM (pulse length), PFM (pulse frequency)
  - Current output (0/4 ... 20 mA): analogue signal to control actuator (for one or two actuator drives)

Valves for position feedback or feedforward control can also be included in the control system. For this, you can use the following optional inputs:

- Order version CXM153-xxx2xxxxx: 1 current input (Ex or non-Ex)
- Order version CXM153-xxx4xxxxx: 2 current inputs (Ex or non-Ex)
- Order version CXM153-xxx3xxxxx: 1 resistance input (non-Ex)
- Order version CXM153-xxx5xxxxx: 1 current and 1 resistance input (non-Ex)

### Selection aids for control

The following selection aids for online and batch processes help you to select the suitable transmitter version for your process.

PWM = pulse length proportional

PFM = pulse frequency proportional

3-point step = three-point step controller

Selection aid for online processes						
Process	Path	Dosing actuators	Required hardware equipment for control			
			Circuits	Relay	Current inputs	Current outputs
1-sided control	looking-ahead · 2-circuit · flow	1 PWM	2	1	1	–
		1 PFM	2	1	1	–
		1 3-point step	2	2	2	–
		1 PWM/PFM	2	2	1	–
		analogue	2	–	1	1
	not looking-ahead	1 PWM	1	1	–	–
		1 PFM	1	1	–	–
		1 3-point step	1	2	1	–
		1 PWM/PFM	1	2	–	–
		analogue	1	–	–	1

C07-CPM153xx-16-12-40-en-002.eps

### Selection aid for online processes

Process	Path	Dosing actuators	Required hardware equipment for control			
			Circuits	Relay	Current inputs	Current outputs
1-sided control	looking-ahead · 2-circuit · flow	1 PWM	2	1	1	—
		1 PFM	2	1	1	—
		1 3-point step	2	2	2	—
		1 PWM/PFM	2	2	1	—
		analogue	2	—	1	1
	not looking-ahead	1 PWM	1	1	—	—
		1 PFM	1	1	—	—
		1 3-point step	1	2	1	—
		1 PWM/PFM	1	2	—	—
		analogue	1	—	—	1

C07-CPM153xx-16-12-00-en-001.epi

### Selection aid for batch processes or slow online processes

Process		Dosing actuators	Required hardware equipment for control			
			Circuits	Relays	Current inputs	Current outputs
1-sided control		1 PWM	1	1	—	—
		1 PFM	1	1	—	—
		1 3-point step	1	2	1	—
		1 PWM/PFM	1	2	—	—
		current output	1	—	—	1
2-sided control		2 PWM	1	2	—	—
		2 PFM	1	2	—	—
		1 3-point step	1	—	1	1
		1 PWM/PFM	1	3	—	—
		current output split range	1	3	—	—

C07-CPM153xx-16-12-00-en-003.epi

### DAT module

The DAT module is a memory device (EEPROM) which is plugged into the terminal compartment of the transmitter.

Using the DAT module, you can:


- **save** complete settings, logbooks and the logged data of the data logs of the Mycom S
- **copy** the complete settings to other Mycom S transmitters which have identical hardware functions.

This considerably reduces the effort to install or service several measuring points.

### Offline configuration with Parawin

Using the **Parawin** PC tool, you can:

1. Configure the whole measuring point on the PC in the familiar Windows environment.
2. Save the settings to the DAT module.
3. Plug the DAT module into a Mycom S and transfer the entire configuration to the transmitter (= complete transmitter setup). Then you can set up other transmitters with the same configuration.
4. You can also use the DAT module to copy logbooks and data logs from the transmitter and to your computer for documentation purposes. You can then display the logged data in graphic form on your PC.

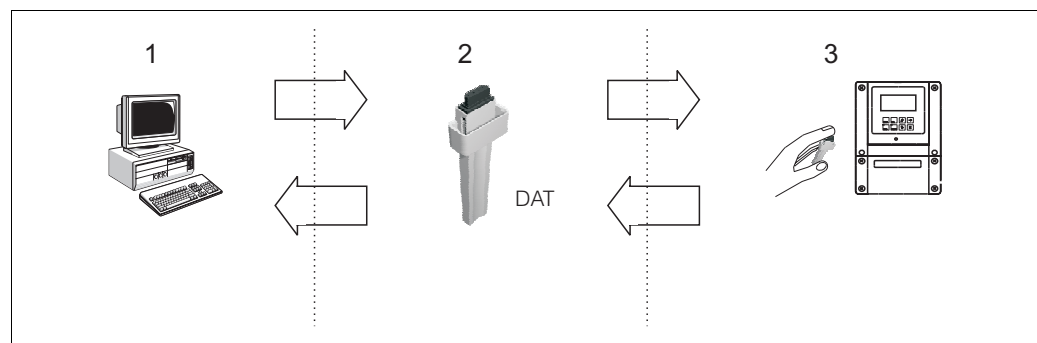

Offline configuration with Parawin (1 - 2 - 3)

Offline data storage (3 - 2 - 1) ⇔

### Calibration and measurement

Calibration options:

- **Airset**  
With inductive sensors the residual coupling between transmitter and detector coil can be compensated by calibration on air.
- **Calculation**  
The conductivity of the calibration solution (with precisely determined conductivity) is entered and the cell constant of the sensor is thus calculated.
- **Installation factor**  
In tight installation conditions, the inductive sensor can be influenced by the pipe wall. This means that measuring differences may occur. These are compensated for in the calibration process by entering an installation factor.
- **Data entry**  
The cell constant of the sensor is entered via the keypad.
- **Calibration logbook**  
The data of the last 30 calibrations are saved to a list with date and time.

Accurate measurement through:

- **Medium temperature compensation (alpha value compensation)**  
This allows high-accuracy measurement over wide temperature ranges. This compensation type compensates the temperature influence on the pH value of the medium.  
Types of compensation:
  - linear compensation
  - NaCl acc. to IEC 746-3
  - neutral ultra pure water (NaCl)
  - acid ultra pure water (HCl)
  - user defined tables

## Input

Measured variable	conductivity, resistivity, temperature			
Measuring range	Inductive conductivity			
		Measuring range		
	not compensated	0.04 μS/cm to 2000 mS/cm		
	compensated	0.04 μS/cm to 1000 mS/cm		
	Conductive conductivity			
	Cell constant k	Measuring range	Display range	
	0.01 cm <sup>-1</sup>	0.0 nS/cm to 600.0 μS/cm	0.0 μS/cm to 200.0 μS/cm	
	0.10 cm <sup>-1</sup>	0.000 μS/cm to 6000 μS/cm	0.000 μS/cm to 2000 μS/cm	
	1.00 cm <sup>-1</sup>	0.00 μS/cm to 60.00 mS/cm	0.00 μS/cm to 20.00 mS/cm	
	10.0 cm <sup>-1</sup>	0.0 μS/cm to 600.0 mS/cm	0.0 μS/cm to 200.0 mS/cm	
Resistivity	Resistivity			
	Cell constant k	Measuring range	Display range	
	0.01 cm <sup>-1</sup>	20.0 kΩ cm to 80.0 MΩ cm	20.0 kΩ cm to 37.99 MΩ cm	
	0.10 cm <sup>-1</sup>	2.00 kΩ cm to 2000 kΩ cm	2.00 kΩ cm to 3799 kΩ cm	
	1.00 cm <sup>-1</sup>	0.200 kΩ cm to 200.0 kΩ cm	0.200 kΩ cm to 379.9 kΩ cm	
	Temperature			
	-35 to +250 °C (-32 to +482 °F)			
	Sensor input	<div>⚠ Sensor circuit with type of protection EEx ia IIC (optional). This circuit may also be connected to sensors of category 1G (zone 0).</div> <div>Maximum output voltage U<sub>O</sub>: DC 12.6 V</div> <div>Maximum output current I<sub>O</sub>: 21 mA</div> <div>Maximum output P<sub>O</sub>: 108 mW</div> <div>Maximum äußere capacity C<sub>O</sub>: 50 nF</div> <div>Maximum äußere inductivity L<sub>O</sub>: 100 μH</div>		
	Current inputs 1/2 (passive, optional)	Signal range:	4 to 20 mA	
		Input voltage range:	6 to 30 V	
	<div>⚠ Intrinsically safe current inputs for connection to intrinsically safe electric circuits with type of protection EEx ia IIC or EEx ib IIC (optional)</div> <div>Maximum input voltage U<sub>i</sub>: DC 30 V</div> <div>Maximum input current I<sub>i</sub>: 100 mA</div> <div>Maximum input P<sub>i</sub>: 3 W</div> <div>Maximum innere capacity C<sub>i</sub>: 1.1 nF</div> <div>Maximum inner inductivity L<sub>i</sub>: 24 μH</div>			
	Resistance input (active, optional, non-Ex only)	Resistance ranges (selectable by the software):	0 to 1 kΩ 0 to 10 kΩ	
Temperature input	connectable temperature sensors:	Pt100 (three wire circuit) Pt1000 NTC 30k		
Binary inputs	Input voltage:	10 to 50 V		
	Inner resistance:	R <sub>i</sub> = 5 kΩ		
	<div>⚠ Intrinsically safe optoelectronic coupler for connection with intrinsically safe electric circuits with type of protection EEx ia IIC or EEx ib IIC</div> <div>Maximum input voltage U<sub>i</sub>: DC 30 V</div> <div>Maximum inner capacity C<sub>i</sub>: negligible</div> <div>Maximum inner inductivity L<sub>i</sub>: negligible</div>			

## Output

Output signal	0/4 to 20 mA	
Signal on alarm	2.4 or 22 mA in case of an error	
Load	maximum 600 Ω (dependent from operating voltage)	
Linearisation transmission behaviour	linear, bilinear, table	
Galvanic isolation	<p>Following circuits are at the same potential:</p> <ul style="list-style-type: none"><li>■ Current output 1 and auxiliary voltage</li><li>■ Current output 2 and resistance input</li></ul> <p>The remaining circuits are galvanically isolated from each other.</p>	
Output distribution	Temperature measurement	
		output distribution: 17 to 170 °C (63 to 338 °F)
	Conductivity measurement	
	measuring range:	output distribution:
	0 to 19.99 μS/cm	2 to 19.99 μS/cm
	20 to 199.9 μS/cm	20 to 199.9 μS/cm
	200 to 1999 μS/cm	200 to 1999 μS/cm
	2 to 19.99 mS/cm	2 to 19.99 mS/cm
	20 to 2000 mS/cm	20 to 2000 mS/cm
	Resistivity measurement	
measuring range:	output distribution:	
0 to 199.9 kΩ·cm	20 to 199.9 kΩ·cm	
200 to 1999 kΩ·cm	200 to 1999 kΩ·cm	
2 to 19.99 MΩ·cm	2 to 19.99 MΩ·cm	
20 to 200 MΩ·cm	20 to 200 MΩ·cm	
Concentration measurement		
	no minimum spacing	
Intrinsically safe signal circuit	<div>Ⓔx</div> <p>Intrinsically safe current output for connection with intrinsically safe electric circuits with type of protection EEx ib IIC</p>	
	Maximum input voltage U <sub>i</sub> :	DC 30 V
	Maximum input current I <sub>i</sub> :	100 mA
	Maximum input P <sub>i</sub> :	750 mW
	Maximum innere capacity C <sub>i</sub> :	negligible
	Maximum inner inductivity L <sub>i</sub> :	negligible
Power supply for binary inputs E1 – E3	Output voltage:	15 V DC
	Output current:	max. 9 mA
	<div>Ⓔx</div> <p>Intrinsically safe current output circuit with type of protection EEx ib IIC</p>	
	Maximum output voltage U <sub>O</sub> :	DC 15.8 V
	Maximum output current I <sub>O</sub> :	71 mA
	Maximum output P <sub>O</sub> :	1.13 W
	Maximum outer capacity C <sub>O</sub> :	50 nF
	Maximum outer inductivity L <sub>O</sub> :	100 μH



**Output relay**

Switching voltage:	max. 250 V AC / 125 V DC
Switching current:	max. 3 A
Switching power:	max. 750 VA
Life span:	≥ 5 million switching cycles



Intrinsically safe relay contact circuits for connection with intrinsically safe electric circuits with type of protection EEx ia IIC or EEx ib IIC

Maximum input voltage $U_i$ :	DC 30 V
Maximum input current $I_i$ :	100 mA
Maximum input $P_i$ :	3 W
Maximum inner capacity $C_i$ :	1.1 nF
Maximum inner inductivity $L_i$ :	24 $\mu$ H

---

**Output controller**

Function (selectable):	Pulse-length controller (PWM) Pulse-frequency controller (PFM) Three-point step-controller (3-point step) Analogue (via current output)
Controller behaviour:	P / PI / PID
Control gain $K_R$ :	0,01 to 20.00
Integral action time $T_n$ :	0,0 to 999.9 min
Derivative action time $T_v$ :	0,0 to 999.9 min
Max. frequency with pulse-frequency controller:	120 min <sup>-1</sup>
Max. period with pulse-length controller:	1 to 999.9 s
Minimum switch-on period with pulse-length controller:	0.4 s


---

**Limit value and alarm functions**

Setpoint adjustments:	0 to 100 % of display range
Hysteresis for switching contacts:	1 to 10 % of display range
Alarm delay:	0 to 6000 s


## Power supply

### Electrical connection

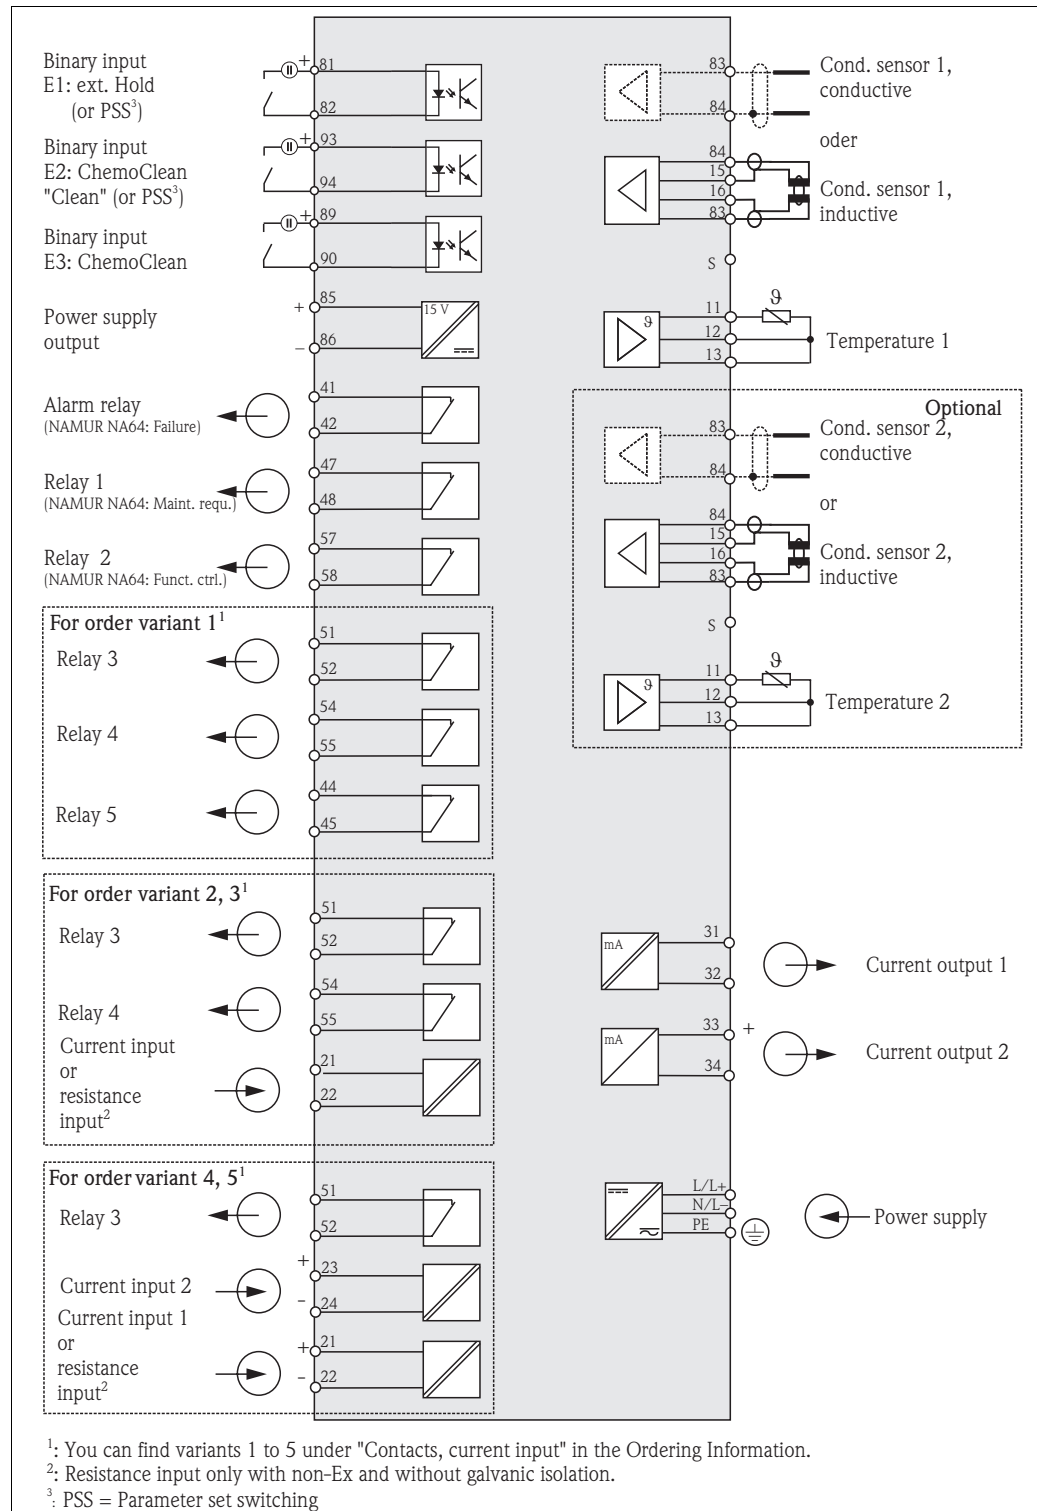











007-CLM153a x-04-06-en-001.eps

Switching example for binary inputs

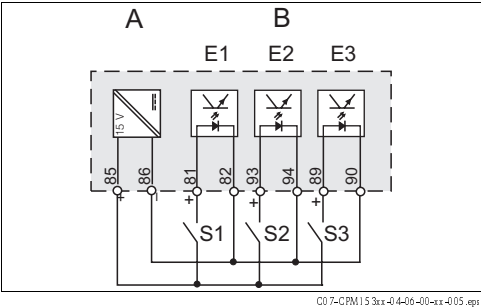

- A Auxiliary voltage output
- B Binary inputs
- E1 External hold
- E2 Chemoclean "Clean"
- E3 Chemoclean "User"
- S1 External de-energised contact
- S2 External de-energised contact
- S3 External de-energised contact

Supply voltage	Version CLM153-xxxx0xxxx Version CLM153-xxxx8xxxx	100 to 230 V AC +10/-15 % 24 V AC/DC +20/-15 %																
Cable specification	Maximum cable cross-section:	2.5 mm <sup>2</sup> (0.0036 sq. inch)																
Power consumption	maximum 10 VA																	
Isolation between galvanically separated current circuits	276 V <sub>eff</sub>																	
Interface connection data	<p>The basic version of Mycom S has one alarm and two additional contacts.</p> <p>The transmitter can be upgraded with the following additional equipment:</p> <ul style="list-style-type: none"><li>■ 3 contacts</li><li>■ 2 contacts and 1 current or resistance input (the latter for non-Ex only)</li><li>■ 1 contact, 1 current input and 1 current or resistance input (the latter for non-Ex only)</li></ul> <p>You can assign functions to the available contacts via the software. The "Active open" and "Active closed" contact types can also be switched by the software.</p> <p>With the appropriate instrument version, you can assign up to three relays to the controller.</p> <p> <b>Note!</b></p> <p>If you use NAMUR contacts (acc. to recommendations of the association for process control engineering of the chemical and pharmaceutical industry), the contacts are set to the relays as follows:</p> <table><tr><th>Relay</th><th>Assignment NAMUR on</th><th>Assignment NAMUR off</th><th>Terminal</th></tr><tr><td>ALARM</td><td>Failure</td><td>Alarm</td><td>41 42 </td></tr><tr><td>RELAY 1</td><td>Warning when maintenance required</td><td>free connectable</td><td>47 48 </td></tr><tr><td>RELAY 2</td><td>Function check</td><td>free connectable</td><td>57 58 </td></tr></table>		Relay	Assignment NAMUR on	Assignment NAMUR off	Terminal	ALARM	Failure	Alarm	41 42 	RELAY 1	Warning when maintenance required	free connectable	47 48 	RELAY 2	Function check	free connectable	57 58 
Relay	Assignment NAMUR on	Assignment NAMUR off	Terminal															
ALARM	Failure	Alarm	41 42 															
RELAY 1	Warning when maintenance required	free connectable	47 48 															
RELAY 2	Function check	free connectable	57 58 															

Frequency	47 to 64 Hz
-----------	-------------

## Performance characteristics

<b>Reference temperature</b>	25 °C (77 °F), settable with medium temperature compensation	
<b>Measured value resolution</b>	Conductivity: Temperature:	0.001 µS/cm 0.1 K
<b>Maximum measured error<sup>a</sup></b>	Display: conductivity, resistivity, concentration: Temperature Current outputs:  Current inputs: Resistance input:	±0.5 % of measured value ±2 digits < 0.5 K max. 0.2 % of current range end value additionally to the display error max. 1 % of measuring range max. 1 % of measuring range
<b>Repeatability<sup>a</sup></b>	Conductivity, resistivity, concentration: Temperature:	±0.2 % of measured value ±2 digits max. 0.1 % of measuring range


## Installation

### Wall mounting



#### Caution!

- Check that the temperature does not exceed the maximum permitted operating temperature range (-20 ... +60 °C / -4 ... 140 °F). Install the instrument in a shady location. Avoid direct sunlight.
- Always install the transmitter so that the cable entries point downwards.

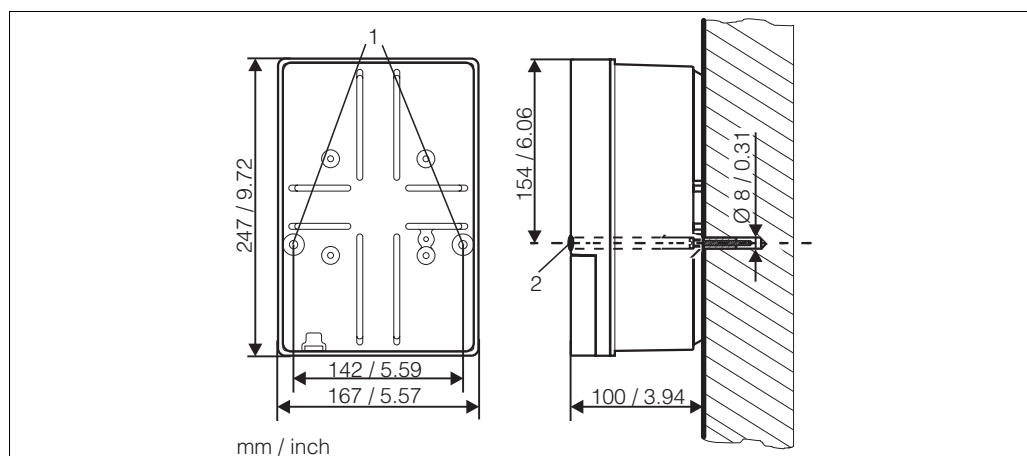


Dimensions for wall mounting, fixing screw: Ø 6 mm / 0.24", wall plug: Ø 8 mm / 0.31"

- 1 Fixing drill holes  
2 Plastic cover cap

a) acc. to IEC 746-1, at nominal operating conditions

## Post mounting and panel mounting

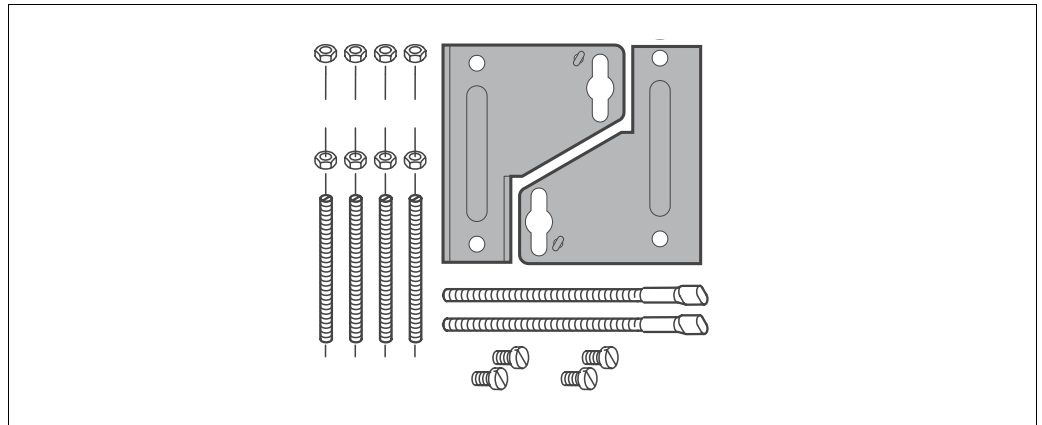

Mounting kit

Mount the parts of the mounting kit at the back of the housing as shown in the figure below.

### Panel mounting:


If you need to seal the front panel mounting of the Mycom S air-tight, you must use an additional flat gasket (see accessories).

Required installation cutout: 161 x 241 mm / 6.34 x 9.41 inches

Installation depth: 134 mm / 5.28"

### Post mounting:

Post diameter: max. 70 mm / 2.76"

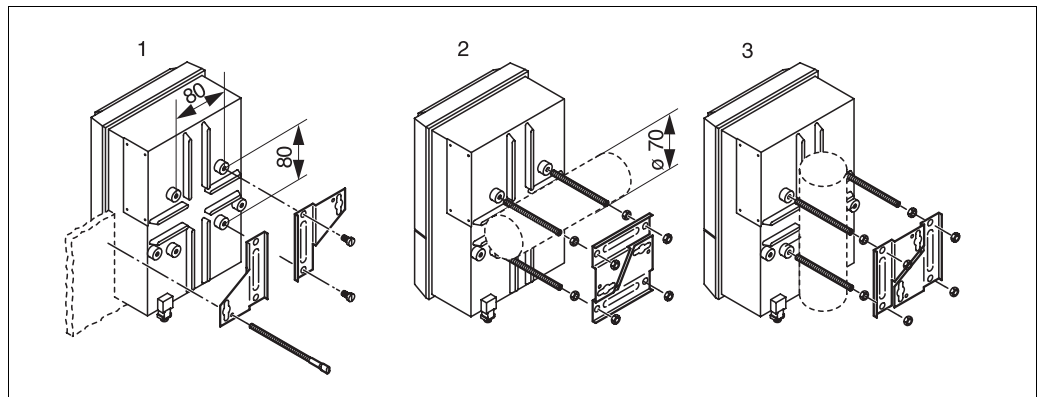


Panel mounting and post mounting

- 1 Panel mounting
- 2 Horizontal post mounting
- 3 Vertical post mounting



### Caution!

Always use the CYY101 weather protection cover for outdoor installation (see figure below and accessories).

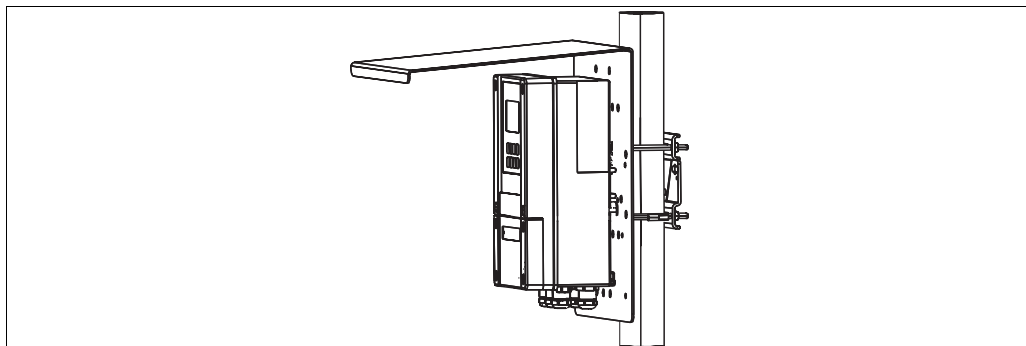

C07-CRM153xx-11-00-01-xx-001.eps


Post mounting with weather protection cover

## Environment

<b>Ambient temperature</b>	-10 ... +55 °C / 14 ... 131 °F (Ex: -10 ... +50 °C / 14 ... 122 °F)
<b>Ambient temperature limit</b>	-20 ... +60 °C / -4 ... 140 °F (Ex: -10 ... +50 °C / 14 ... 122 °F)
<b>Relative humidity</b>	10 ... 95%, non-condensing
<b>Storage temperature</b>	-30 ... +80 °C / -22 ... 176 °F
<b>Ingress protection</b>	IP 65
<b>Electromagnetic compatibility</b>	Interference emission acc. to EN 61326: 1997 / A1: 1998, class B resources (housing sector) Interference emission acc. to EN 61326: 1997 / A1: 1998, appendix A (industrial sector)

## Mechanical construction

### Design, dimensions

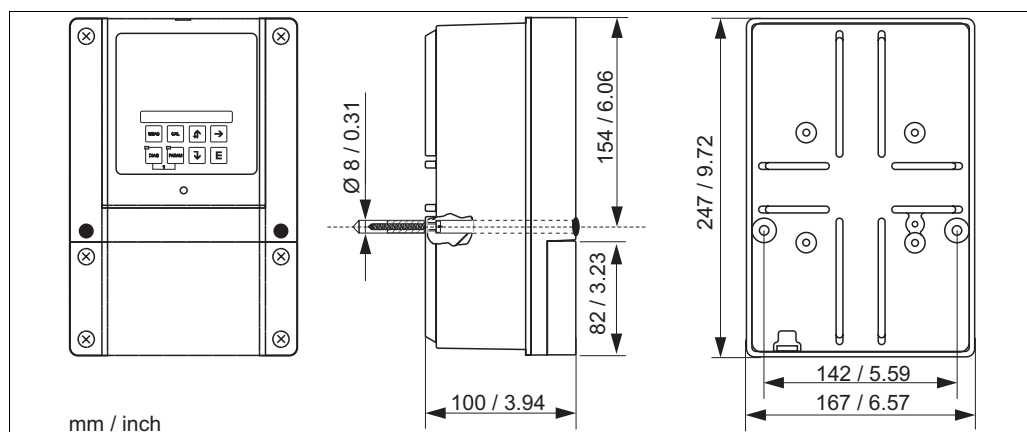

C07-CRM15340-00-00-en-001.eps

<b>Weight</b>	maximum 6 kg (13.2 lb)
---------------	------------------------


<b>Materials</b>	Housing: Front:	GD AlSi 12 (Mg content 0.05 %), plastic coated polyester, UV resistant
------------------	--------------------	---

## Human Interface

### Display and operating elements

Backlit LC display with dot matrix, 128 x 64 dots

The display shows the current measured value and the temperature, i.e. the most important process data, at a glance. In the configuration menu, online help pages help you to enter suitable instrument parameters.

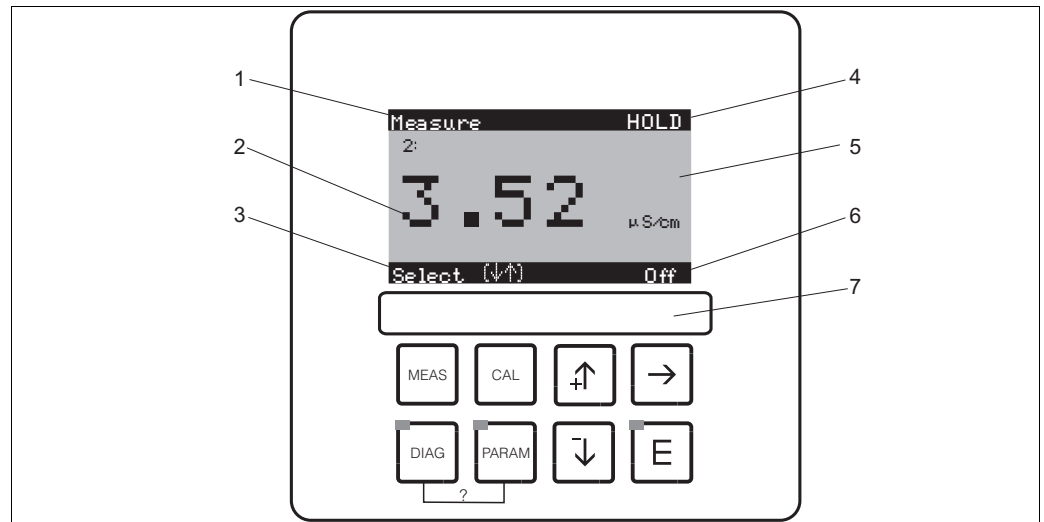

- |   |   |       |                                    |
|---|---|-------|------------------------------------|
| 1 | Current menu  | MEAS  | Measuring mode key                 |
| 2 | Current parameter   | CAL   | Calibration mode key               |
| 3 | Navigation bar: arrow keys for scrolling; "E" for browsing; note for cancelling | DIAG  | Diagnosis mode key                 |
| 4 | HOLD display, if active   | PARAM | Parameter entry mode key           |
| 5 | Current main measured value   | →     | Arrow keys for selection and enter |
| 6 | "Failure" display, "Warning" if NAMUR contacts are active                       | ↑     |                                    |
| 7 | Labelling strip   | ↓     |                                    |
| ? | Simultaneously pressing DIAG and PARAM opens the online help                    | E     | Enter key                          |

007-CLM153a-1 9-06-00-en-001.eps

### Operating functions

Four main menus are available for instrument operation:

- Measurement
- Configuration
- Calibration
- Diagnosis

Press the **MEAS**, **PARAM**, **CAL** and **DIAG** keys to switch to the appropriate menu. The submenus are displayed in plain text and the selected elements are displayed in reverse video. Use the arrow keys to select elements and to edit numeric values.

### Access codes

To protect the transmitter from unintended or undesired modification of the configuration and calibration data, four-digit access codes can be defined. Access authorisation has the following levels:

- Read-only level (accessible without code)  
The complete menu can be viewed. The configuration cannot be changed. Calibration is not possible. Only the controller parameters can be changed in the "DIAG" menu branch.
- Maintenance level (can be protected by the service code)  
This code permits calibration.  
Use this code to operate the temperature compensation menu command. The test functions and the internal data can be viewed.
- Specialist level (can be protected by the specialist code)  
All menus are accessible for modification.




Note!

As long as no codes are defined, all functions are freely accessible.

## Remote operation

The PC tool enables you to configure your measuring point offline on a PC using a simple and self-explaining menu structure (see window example below). Write the configuration to the DAT module using the RS232 interface of the PC. The module can then be plugged into the transmitter.

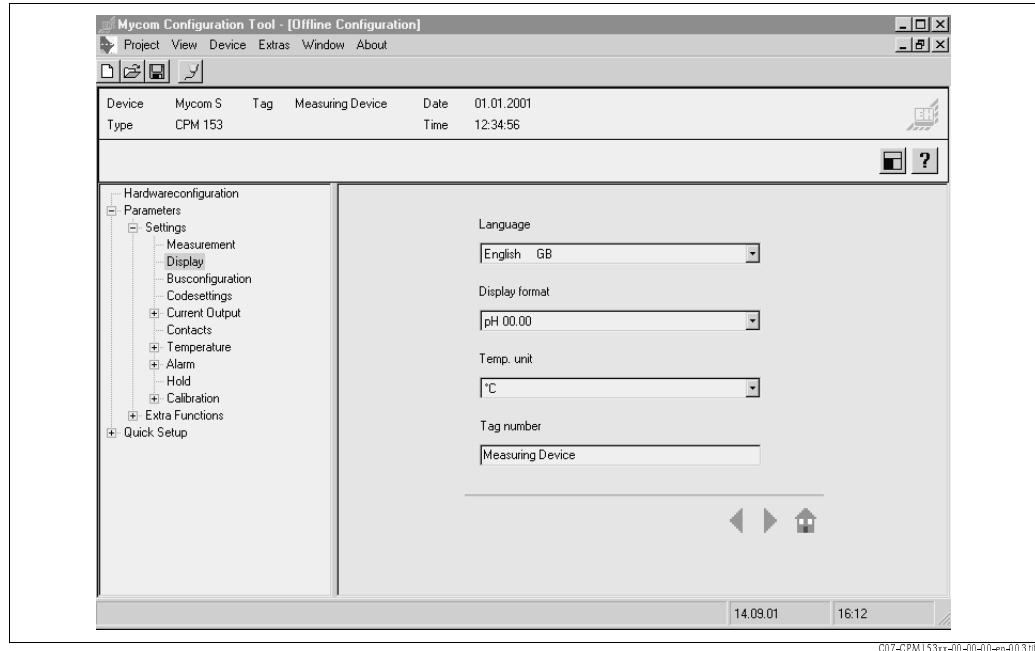

Parawin structure

## Certificates and approvals

### CE symbol

#### Declaration of conformity

The product meets the legal requirements of the harmonised European standards.  
The manufacturer confirms compliance with the standards by affixing the **CE** symbol.

### Ex approval

Depending on ordered version:

- ATEX II (1) 2G, EEx em ia/ib IIC T4
- FM NI Class I, Division 2, Groups A, B, C, D; sensor IS Class I Division 1, Groups A, B, C, D  
FM DIP Class II, III, Division 1, Groups E, F, G; sensor IS Class I Division 1, Groups A, B, C, D
- FM NI Class I, Division 2, Groups A, B, C, D  
FM DIP Class II, III, Division 1, Groups E, F, G
- CSA Class I, Division 2; sensor IS Class I Division 1
- FM IS NI Cl. I, II, III, Div. 1&2, Group A-G
- TIIS



## Ordering information

### Product structure

Certificates									
A									Basic version for non-Ex areas
G									With ATEX approval, ATEX II (1) 2G EEx, em i b l a j IIC T4, only passive current outputs
O									With FM approval, NI Cl. I, Div. 2, Sensor IS Cl. I, Div. 1, only passive current outputs
P									With FM approval, NI Cl. I, Div. 2, only passive current outputs
S									With CSA approval, NI Cl. I, Div. 2, Sensor IS Cl. I, Div. 1, only passive current outputs
T									With TIS approval, only passive current outputs
Sensor inputs									
1									1 measuring circuit for conductive sensors, conductivity/resistivity and temperature
2									1 measuring circuit for inductive sensors, conductivity/resistivity and temperature
3									2 measuring circuits for conductive sensors, conductivity/resistivity and temperature
4									2 measuring circuits for inductive sensors, conductivity/resistivity and temperature
Output signals									
A									2 current outputs 0/4 ... 20 mA, passive (Ex and non-Ex)
B									2 current outputs 0/4 ... 20 mA, active (non-Ex)
C									HART with 2 current outputs 0/4 ... 20 mA, passive (Ex and non-Ex)
D									HART with 2 current outputs 0/4 ... 20 mA, active (non-Ex)
E									PROFIBUS-PA, no current outputs
Contacts, current inputs									
0									no additional contacts
1									3 additional contacts
2									2 additional contacts, 1 current input passive (Ex and non-Ex)
3									2 additional contacts, 1 resistance input active (non-Ex)
4									1 additional contact, 2 current inputs passive (Ex and non-Ex)
5									1 additional contact, 1 current input passive, 1 resistance input active (non-Ex)
Power supply									
0									100 to 230 V AC
8									24 V AC/DC
Languages									
A									E / D
B									E / F
C									E / I
D									E / ES
E									E / NL
F									E / J
Cable entries									
0									Cable glands M 20 x 1.5
1									Cable entry NPT 1/2"
3									Cable gland M 20 x 1.5, PROFIBUS-PA-M12 plug
4									Cable gland NPT 1/2", PROFIBUS-PA-M12 plug
Additional features									
0									Standard version
1									DAT module
Configuration									
0									Factory setup
CLM153-									complete order code

### Scope of delivery


The scope of delivery comprises:

- 1 transmitter
- 1 mounting kit
- 4 cable glands
- 1 set for measuring point labelling
- 1 instrument identification card
- 1 Operating Instructions english
- Versions with HART communication:
  - 1 Operating Instructions field communication with HART, English
- Versions with PROFIBUS interface:
  - 1 Operating Instructions field communication with PROFIBUS PA, English
- Ex versions acc. to ATEX:
  - Safety instructions for electrical equipment in explosion hazardous areas, XA 233C/07/a3

## Accessories

### Sensors

- ☐ ConduMax W CLS 12  
Conductive conductivity sensor for standard, Ex and high temperature applications;  
Ordering acc. to version, see Technical Information TI 082/C07/en
- ☐ ConduMax W CLS 13  
Conductive conductivity sensor for standard, Ex and high temperature applications;  
Ordering acc. to version, see Technical Information TI 083/C07/en
- ☐ ConduMax W CLS 15  
Conductive conductivity sensor for pure and ultra-pure water applications (incl. Ex);  
Ordering acc. to version, see Technical Information TI 109/C07/en
- ☐ ConduMax W CLS 16  
Hygienic conductive conductivity sensor for pure and ultra-pure water applications;  
Ordering acc. to version, see Technical Information TI 227/C07/en
- ☐ ConduMax W CLS 19  
Conductive conductivity sensor for pure and ultra-pure water applications;  
Ordering acc. to version, see Technical Information TI 110/C07/en
- ☐ ConduMax W CLS 21  
Conductive conductivity sensor for applications with middle to high conductivity  
(incl. Ex); Ordering acc. to version, see Technical Information TI 085/C07/en

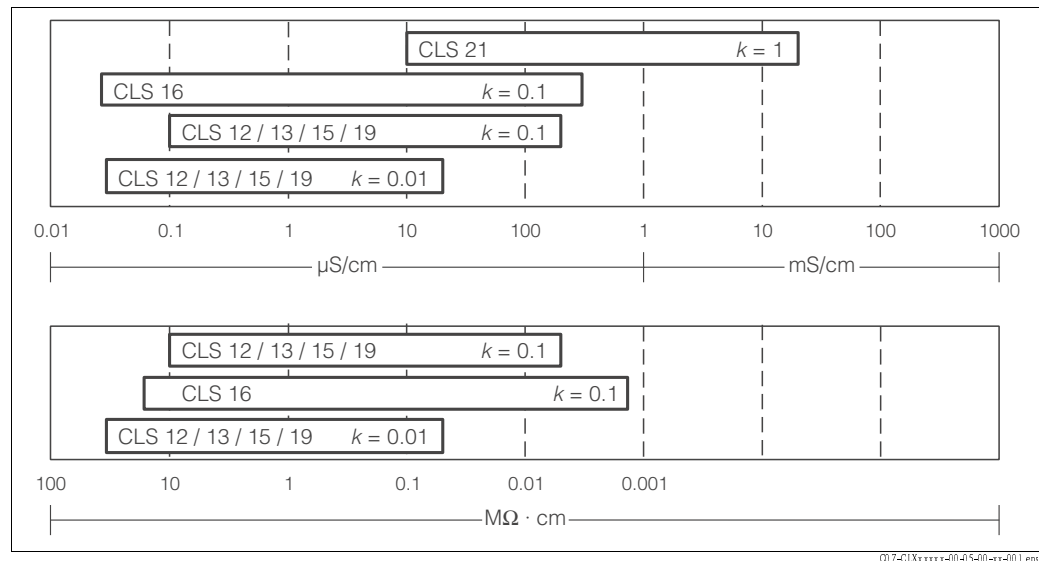

Application ranges of conductive conductivity sensors:

top = conductivity

bottom = specific resistance


- ☐ InduMax P CLS 50  
Inductive conductivity sensor for standard, Ex and high temperature applications;  
Ordering acc. to the sensor version, see Technical Information (order no. 50090385)
- ☐ InduMax H CLS 52  
Inductive conductivity sensor with short response time in hygienic design;  
Ordering acc. to the sensor version, see Technical Information (order no. 50086110)

### Assemblies (selection)


- ☐ DipFit W CLA 111  
Immersion assembly for open and closed tanks with flange DN 100;  
Ordering acc. to version, see Technical Information
- ☐ DipFit P CLA 140  
Immersion assembly with flange connection for high duty processes;  
Ordering acc. to the version, see Technical Information (order no. 51500081)
- ☐ Immersion assembly Dipfit W CYA611  
for sensor immersion in basins, open channels and tanks, PVC;  
Ordering acc. to product structure (Technical Information TI 166C/07/en)

**Mounting accessories**

- ☐ Weather protection cover CYY101 for mounting of field housing, for outdoor installation  
material: stainless steel 1.4031;  
order no. CYY101-A

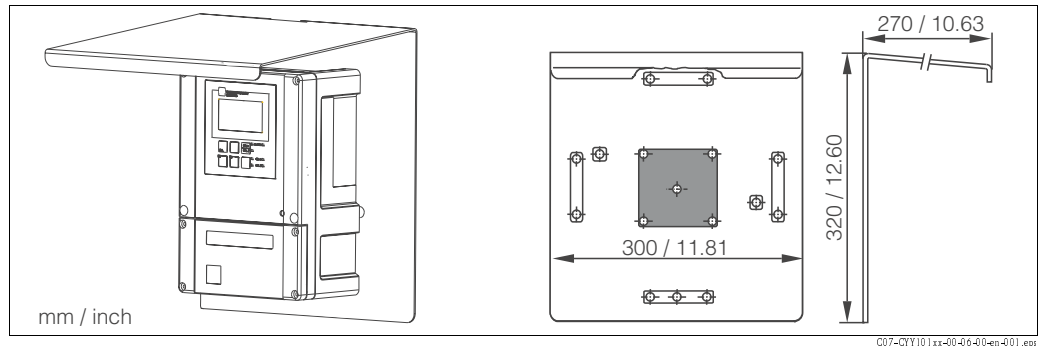*Weather protection cover for field instrument*

- ☐ Round post fixture to fix the weather protection cover to vertical or horizontal posts with diameters of up to 70 mm / 2.76";  
Order no. 50062121

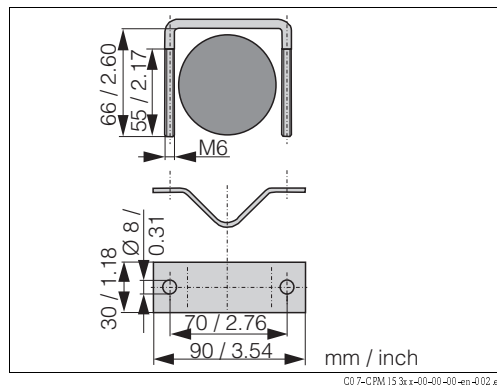*Round post fixture for CYY101***Connection accessories**

- ☐ CPK9 special measuring cable  
For sensors with TOP68 plug-in head, for high-temperature and high-pressure applications, IP 68  
Ordering acc. to product structure, see Technical Information (TI 118C/07/en)
- ☐ Extension cable CLK 5  
for inductive conductivity sensors, for cable extension via junction box VBM;  
(ordering per meter), order no. 50085473
- ☐ CYK 71  
for conductive conductivity sensors, for cable extension via VBM junction box;  
order no. 50085333
- ☐ CYK 71-Ex  
for Ex applications, like CYK 71, but blue cable sheath;  
order no. 50085673
- ☐ Junction box VBM  
for cable extension, with 10 terminals, IP 65 / NEMA 4X

Cable entry Pg 13.5

Order no. 50003987

Cable entry NPT 1/2"

Order no. 51500177

**DAT module**

- ☐ Additional memory device for saving or copying complete settings, logbooks and the data logs;  
Order no.: 51507175

**Flat gasket**

- ☐ Flat gasket for sealing the front panel mounting of the Mycom S  
Order no.: 50064975

## Offline configuration with Parawin

### ☐ Parawin

Graphical PC software for offline configuration of the measuring point at the PC. The language is selectable. Required operating systems: Windows NT/95/98/2000.

The offline configuration tool consists of:

- a DAT module
- DAT interface (RS 232)
- Software

Order no.: 51507133 (Mycom S only)

Order no.: 51507563 (Topcal S, Topclean S, Mycom S)

## Documentation

### Operating Instructions

- ☐ Operating Instructions Mycom S CLM153, BA234C/07/en, order no. 51503794
- ☐ Ex Safety Instructions, XA233C/07/a3, order no. 51506728
- ☐ Operating Instructions PROFIBUS-PA/-DP, BA298C/07/en, order no. 51507116
- ☐ Operating Instructions HART, BA301C/07/en, order no. 51507114

### Conductive conductivity

- ☐ Condumax W CLS12, Technical Information, TI 082C/07/en; order no. 50059349
- ☐ Condumax W CLS13, Technical Information, TI 083C/07/en; order no. 50059350
- ☐ Condumax W CLS15, Technical Information, TI 109C/07/en; order no. 50065950
- ☐ Condumax W CLS16, Technical Information, TI 227C/07/en; order no. 51503431
- ☐ Condumax W CLS19, Technical Information, TI 110C/07/en; order no. 50065951
- ☐ Condumax W CLS21, Technical Information, TI 085C/07/en; order no. 50059352
- ☐ Dipfit W CLA111, Technical Information TI 135C/07/en; order no. 50076858

### Inductive conductivity

- ☐ Indumax P CLS50, Technical Information, TI 182C/07/en; order no. 50090385
- ☐ Indumax H CLS52, Technical Information, TI 167C/07/en; order no. 50086110
- ☐ Dipfit P CLA140, Technical Information TI 196C/07/en; order no. 51500081

## International Head Quarters

Endress+Hauser  
GmbH+Co. KG  
Instruments International  
Colmarer Str. 6  
79576 Weil am Rhein  
Deutschland

Tel. +49 76 21 9 75 02  
Fax +49 76 21 9 75 34 5  
www.endress.com  
info@ii.endress.com