



Level



Pressure



Flow



Temperature



Liquid  
Analysis



Registration



Systems  
Components



Services



Solutions

## Technical Information

# Stamolys CA71HA

## Total Hardness Analyzer

Compact photometric analysis system for total hardness measurement in drinking water systems



### Application

- Total hardness monitoring in reverse osmosis systems inlets
- Total hardness monitoring after ion exchange systems
- Monitoring of precipitant addition in drinking water treatment plants

### Your benefits


- Direct reaction in photometer at constant temperature
- Fast response time due to low system volume and short distances
- Low reagent requirement
- Low sample requirement
- Two selectable measuring ranges
- User-friendly interface
- Sample stream monitoring and plain text error menu
- Measured value storage using integrated data logger
- Automatic self-cleaning
- Automatic calibration
- With two channel version: measurement sequences programmable
- Two housing versions and an open version available

## Function and system design

### Measuring principle

After sample conditioning, the analyzer sample pump conveys a part of the filtrate to a mixing vessel. The reagent pump adds reagent at a specific ratio. As a result of the reaction, the sample turns a characteristic colour. The photometer determines the sample's absorption of an emitted light at a specific wavelength (s. Fig., Pos. 2). The wavelength is parameter specific. The absorption intensity is proportional to the concentration of the specified parameter in the sample (Pos. 3). Additionally, the absorption of a reference light is determined to receive a genuine measuring result. The reference signal is subtracted from the measuring signal to prevent any effects due to turbidity, contamination and ageing of the LEDs.

The temperature in the photometer is controlled thermostatically so that the reaction is reproducible and takes place within a short period of time.

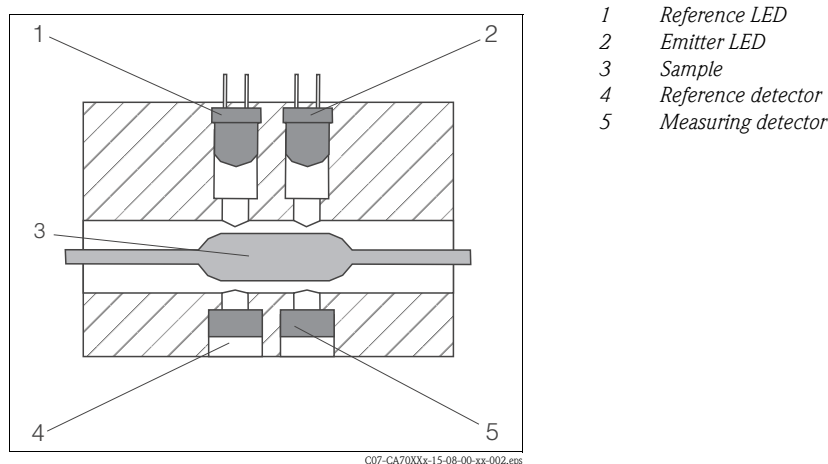

Photometric principle

### Photometric determination

#### Complexometric method for total hardness determination

By adding MgEDTA to the sample, calcium is equivalently replaced by magnesium.

At pH 10 calcium, magnesium and eriochrome black T form a ruby dye.

The absorption is determined at a wavelength of 525 nm (HA-A) resp. 880 nm (HA-B). The absorption intensity is proportional to the total hardness in the sample.

The reference wavelength is 660 nm (HA-A) resp. 740 nm (HA-B).

### Interferences

No interferences up to the given concentration:

Concentration [mg/l]	Ion
2.00	Fe <sup>3+</sup>
1.40	Fe <sup>2+</sup>
0.75	Cu <sup>2+</sup>
0.25	Cr <sup>3+</sup>
0.20	Mn <sup>2+</sup>
0.05	Zn <sup>2+</sup>

## Sample conditioning

### Micro/ultrafiltration (Stamoclean CAT430, optional)

A membrane filter element is suspended directly into the wastewater basin or channel. A hose pump is located in a pump box on the basin rim. The pump creates a vacuum between the membrane and the carrier plate of the filter element. This vacuum makes the filtrate pass through the filter membrane. Suspended materials, particles, algae and bacteria are collected on the surface of the membrane.

Due to alternating pumping and pause, intervals of more than one month are achieved between cleaning cycles. Parallel connection of two or four filter elements increases the sampling quantity up to approx. 1 l/h. The hose pump pressure transports the sample to a collecting vessel near the analyzer over a distance of 20 m. For distances up to 100 m the sample is transported to the collecting vessel by means of compressed air. The analyzers suck the needed sample volume from the collecting vessel.

### Membrane filtration (Stamoclean CAT411, optional)

A sample flow of 0.8 to 1.8 m<sup>3</sup>/h is continuously conducted through the micro filter via a pressure pipe. A part of the sample passes the filter membrane and is then conveyed to the measuring device as filtrate.

Sampling is based on the cross flow filtration principle. The PTFE filter membrane separates particles with sizes > 0.45 µm from the filtrate. These particles are collected in front of the membrane and are washed away with the sample flow.

The medium is conducted in a meander-like channel through the filter element. This results in a constantly high flow rate. The high flow rate generates the self cleaning effect. Therefore, mechanical drives for the generation of a flow at the filter surface are not necessary.

### Backwash filter (Stamoclean CAT221, optional)

A sample flow of 1 to 2.5 m<sup>3</sup>/h is permanently conveyed through the backwash filter by means of a sampling pump or a pressure pipe. The filtrate passes through the wedge wire sieve and is then transported to the measuring device.

Clogging is minimised by the tangential flow of the wedge wire sieve. Automatic backwashing results in a filter operating time of several weeks.

The automatic backwashing and a small compressor guarantee low-maintenance and low-energy operation.

### Customer specific solution


Before analysis, the sample has to be conditioned and to be transported to an external or to the delivered collecting vessel.

## Measuring system

A complete measuring system comprises:


- An analyzer
- A sample conditioning system (optionally):
  - Micro filtration / ultra filtration Stamoclean CAT430 or Stamoclean CAT411
  - Backwash filter Stamoclean CAT221
  - Customer specific solution
- Collecting vessel (see product structure)

### Micro / ultra filtration

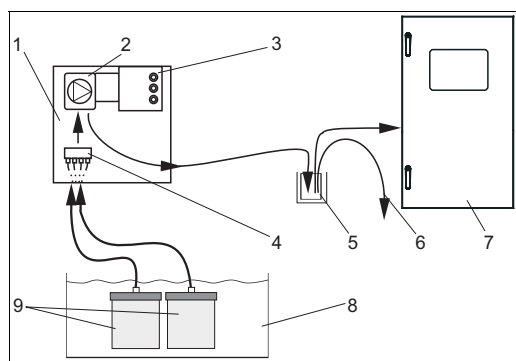

- 1 Hose pump box
- 2 Hose pump
- 3 Control unit
- 4 Collecting unit (optional)
- 5 Collecting vessel
- 6 Overflow
- 7 Analyzer
- 8 Aeration basin
- 9 Membrane filter

Measuring system with Stamoclean CAT430

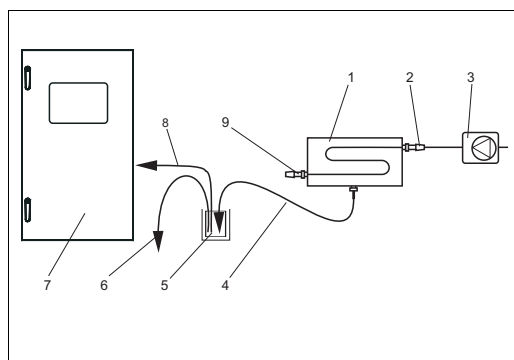


C07-CA71XXc-14-08-00-xx-003.eps

Measuring system with Stamoclean CAT 411

- 1 Stamoclean CAT411
- 2 Inlet
- 3 Sample pump or hydraulic main
- 4 Filtrate line
- 5 Collecting vessel
- 6 Overflow
- 7 Analyzer
- 8 Analyzer sample line
- 9 Outlet

### Backwash filter

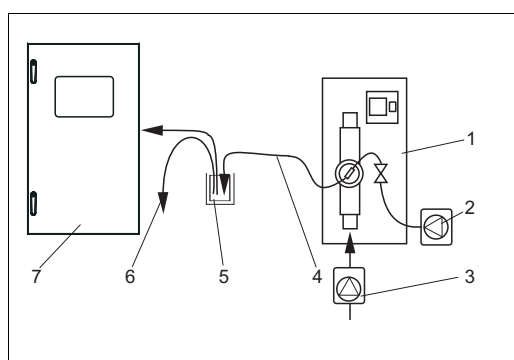

C07-CA70XXc-14-08-00-xx-002.eps

Measuring system with StamoClean CAT 221

- 1 StamoClean CAT 221
- 2 Compressor or compressed air
- 3 Sample pump or hydraulic main
- 4 Sample outlet
- 5 Collecting vessel
- 6 Overflow
- 7 Analyzer

## Input


Measured variable	CaCO <sub>3</sub> [mg/l, °fH, °dH, mmol/l, ppm]
Measuring ranges	0.1 ... 10 mg/l CaCO <sub>3</sub> (HA-A) 0.8 ... 80 mg/l CaCO <sub>3</sub> (HA-B)
Wavelength	525 nm (HA-A) 880 nm (HA-B)
Reference wavelength	660 nm (HA-A) 740 nm (HA-B)

Output

Output signal	0/4 ... 20 mA
Signal on alarm	Contacts: 2 limit contacts (per channel), 1 system alarm contact optional: end of measurement (with two channel version display of channel no. available)
Load	max. 500 Ω
Data interface	RS 232 C
Data logger	1024 data pairs per channel with date, time and measured value 100 data pairs with date, time and measured value for calibration factor determination (diagnostic tool)
Load capacity	230 V / 115 V AC max. 2 A, 30 V DC max. 1 A

Power supply

Electrical connection

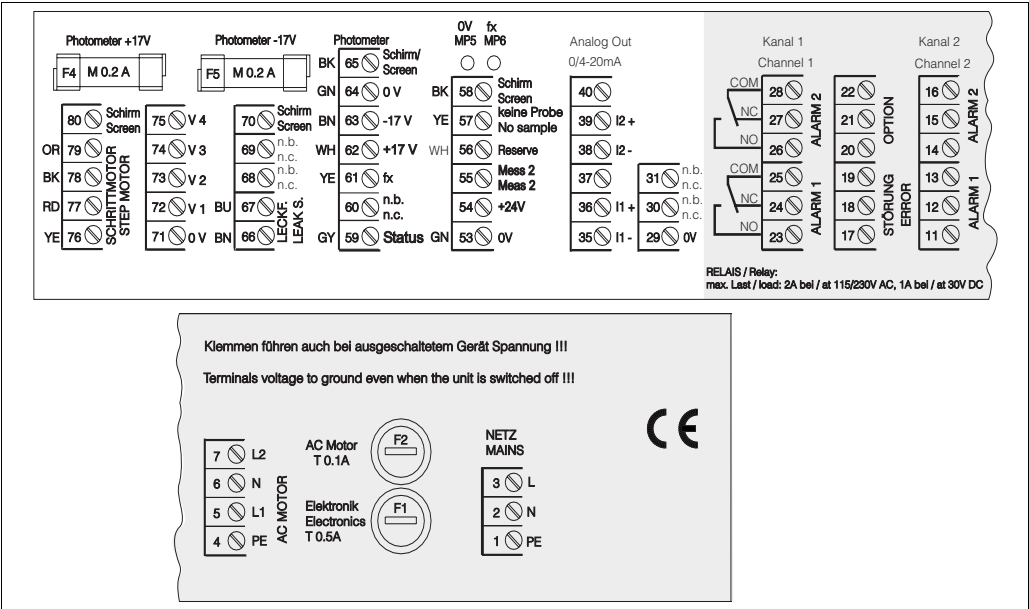

Connection sticker CA 71

Supply voltage	115 V AC / 230 V AC $\pm 10\%$ , 50/60 Hz
Power consumption	approx. 50 VA
Current consumption	approx. 0.2 A at 230 V approx. 0.5 A at 115 V
Fuses	1 x time-lag 0.5 A for electronics 2 x medium time-lag 0.2 A for photometer 1 x time-lag 0.1 A for motors

## Performance characteristics

<b>Time between two measurements</b>	$t_{\text{mes}}$ = reaction time + rinse time + waiting time + rinse again time + filling time + sampling time + reagent refusal time (min. waiting time = 0 min)
<b>Maximum measured error</b>	5 % of measuring range end (HA-A) 3 % of measuring range end (HA-B)
<b>Measuring interval</b>	$t_{\text{mes}}$ to 120 min
<b>Reaction time</b>	2 minutes
<b>Sample requirement</b>	20 ml (0.0053 US.gal.) per measurement
<b>Reagent requirement</b>	2 x 0.1 ml (0.00026 US.gal) 1.0 l (0.264 US.gal) per reagent per 90 days (HA-A) resp. per 21 days (HA-B) with a 10 minute measuring interval
<b>Calibration interval</b>	0 to 72 h
<b>Rinse interval</b>	0 to 72 h
<b>Rinse time</b>	selectable from 20 to 300 s (standard = 80 s)
<b>Rinse again time</b>	60 s
<b>Filling time</b>	15 s (HA-A) 10 s (HA-B)
<b>Sampling time</b>	$t_{\text{sampling}} = 80 \text{ s}$
<b>Reagent refusal time</b>	$t_{\text{refusal}} = 20 \text{ s}$ (HA-A) $t_{\text{refusal}} = 10 \text{ s}$ (HA-B)
<b>Maintenance interval</b>	6 months (typical)
<b>Servicing requirement</b>	15 minutes per week (typical)


## Environment

<b>Ambient temperature</b>	5 ... 40 °C (41 ... 104 °F), avoid strong fluctuations
<b>Humidity</b>	below the condensation limit, installation in usual, clean rooms outdoor installation only possible with protective devices (customer supplied)
<b>Ingress protection</b>	IP 43


Process

Sample temperature	5 to 40 °C (41 to 104 °F)
Sample flow rate	min. 5 ml (0.0013 US.gal.) per min
Consistence of the sample	low solid content (< 50 ppm)
Sample inlet	pressureless
Sample pH value	> pH 3 (not buffered)


Mechanical construction

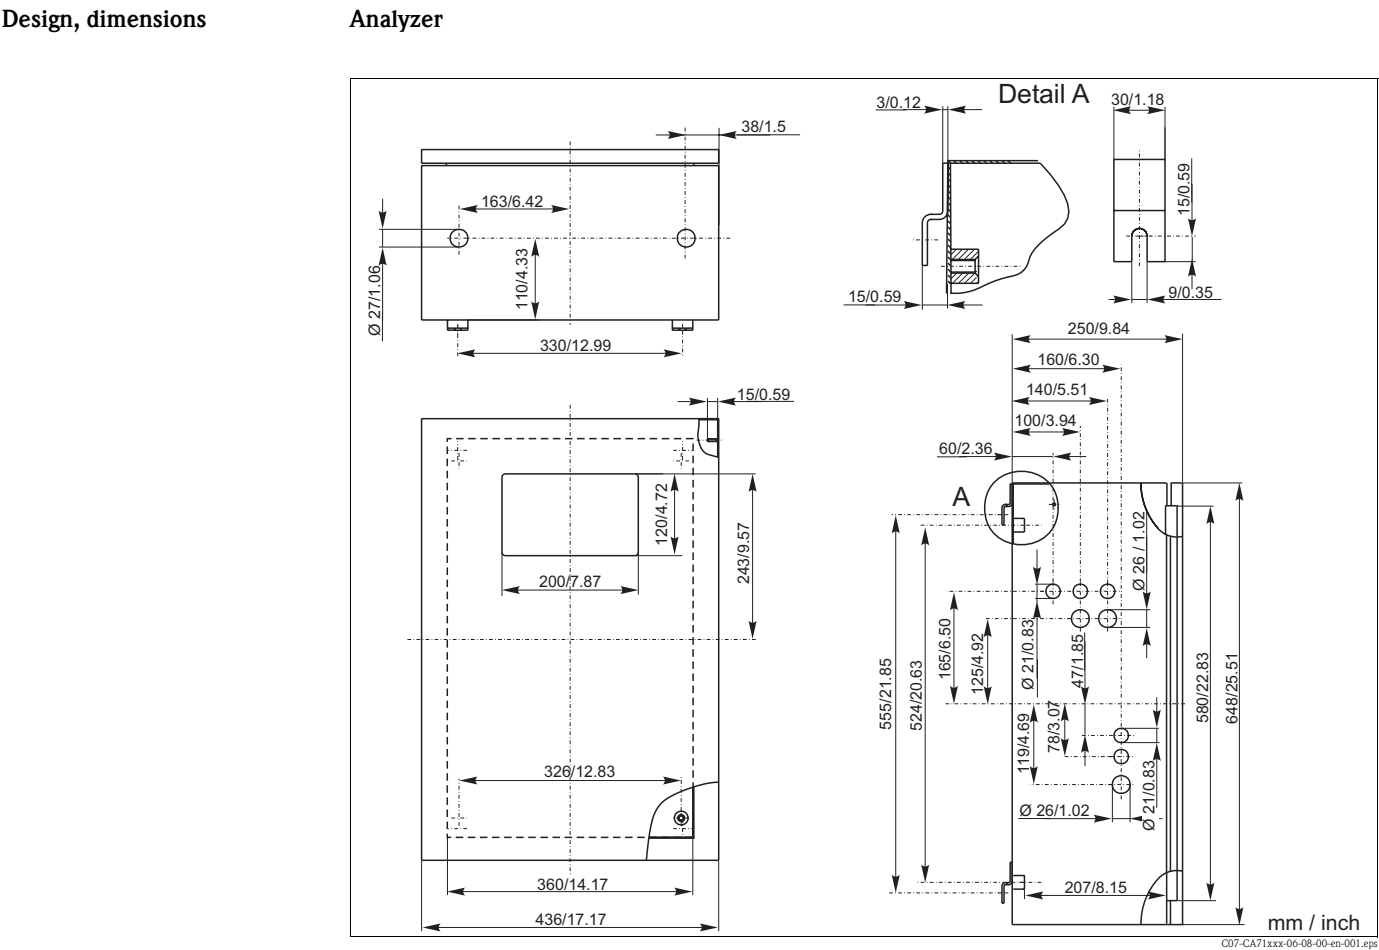

Stainless steel version

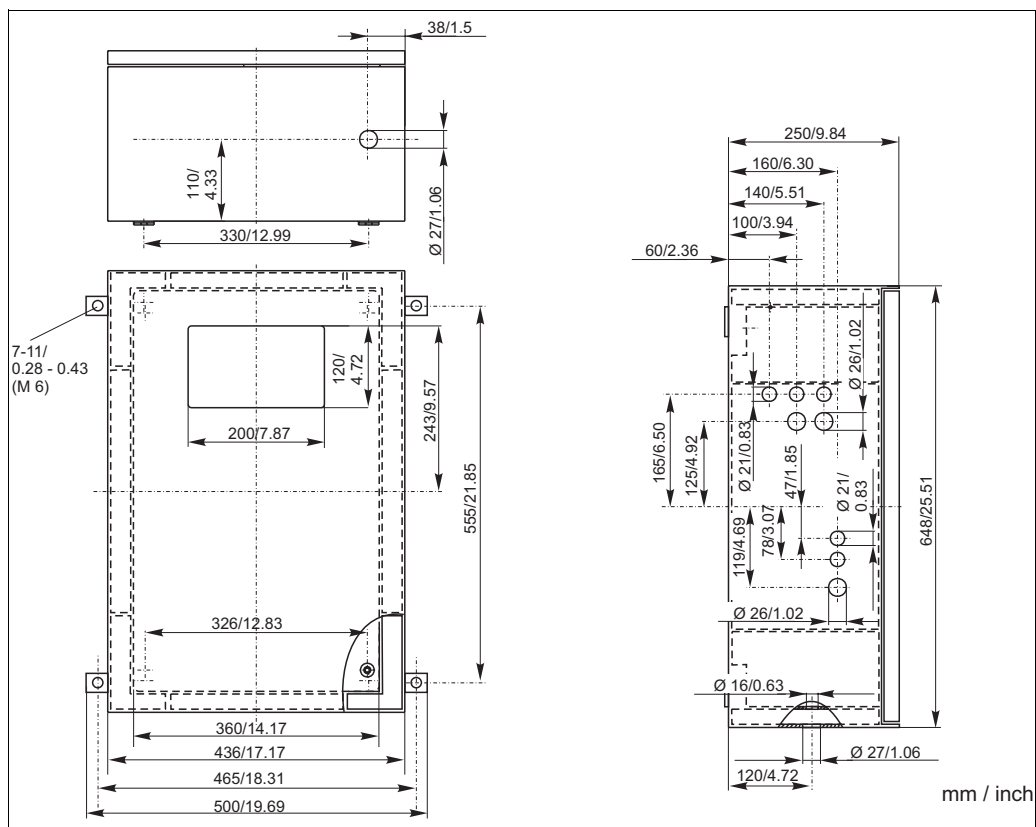


GFK version

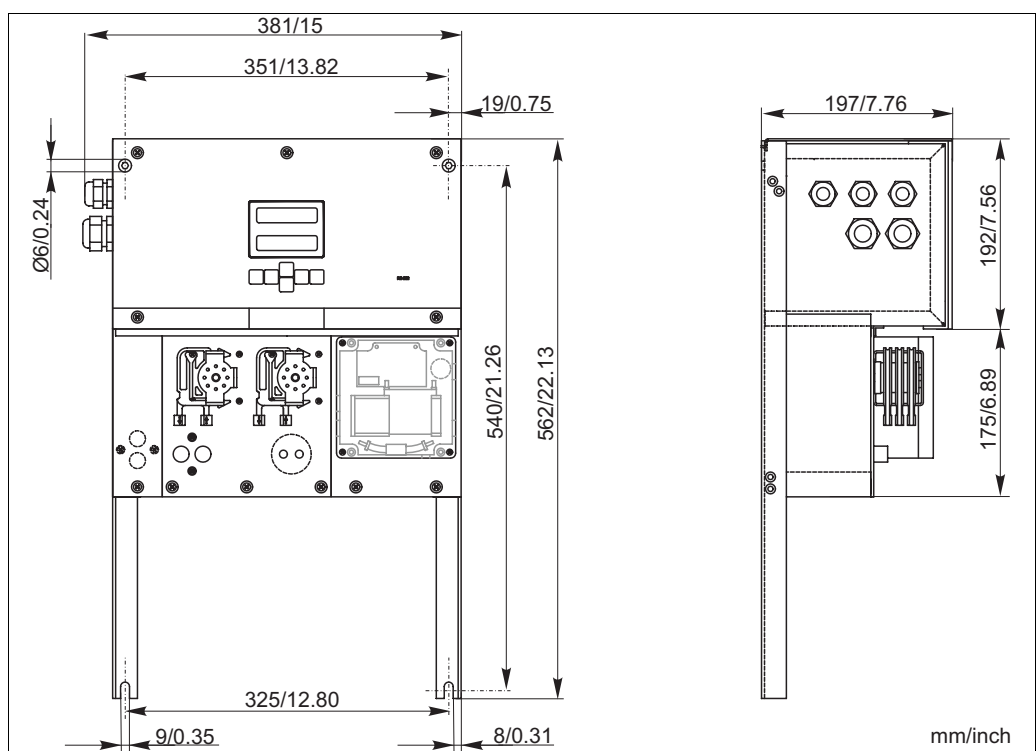

Open version (without housing)




Collecting vessel

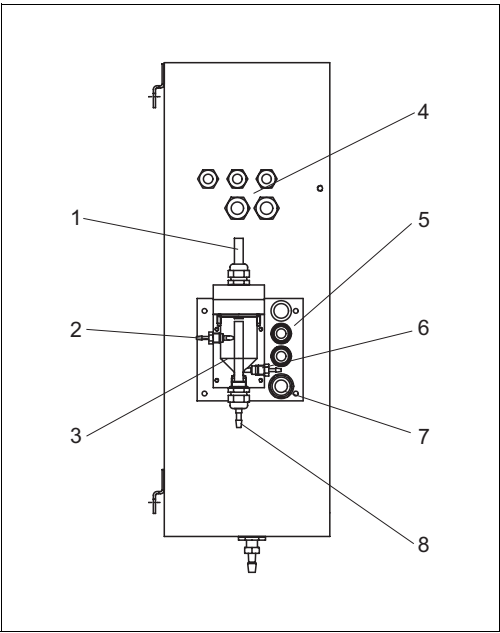

C07-CA71xxx-11-08-00-xx-001.eps

Collecting vessel at analyzer (optional)

- 1 Ventilation
- 2 Sample inlet from sampling
- 3 Collecting vessel
- 4 Electrical connections
- 5 Analyzer sample inlet

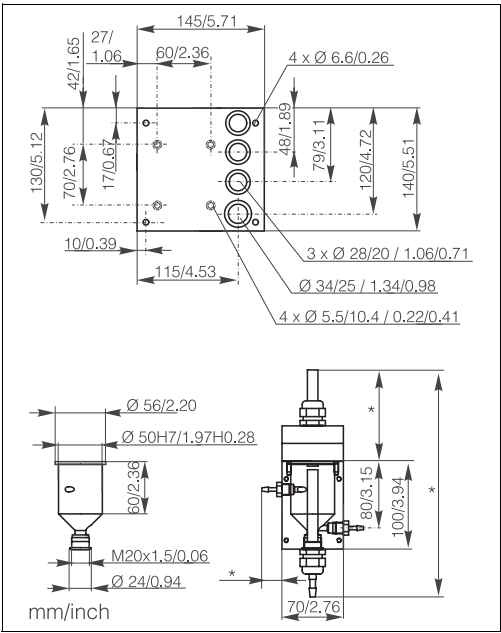

C07-CA71xxx-06-08-02-en-003.eps


Collecting vessel dimensions

- \* variable, freely adjustable dimensions
- 6 Sampling for analyzer
- 7 Analyzer outlet
- 8 Sample overflow

Weight	GFK housing	approx. 28 kg (61.7 lb)
	Stainless steel housing	approx. 33 kg (72.8 lb)
	Without housing	approx. 23 kg (50.6 lb)
Material	Housing:	Stainless steel 1.4301 (AISI 304) or GFK
	Front windows:	Plexiglass®
	Endless hose:	C-Flex®, Norprene®
	Pump hose:	Tygon®, Viton®
	Valves:	Tygon®
Sample line connection	<b>One channel version</b>	
	<i>Collecting vessel</i> (at analyzer, with or without level measurement)	
	Connection	hose ID 3.2 mm (0.13")
	<i>Customer collecting vessel</i>	
	Connection	hose ID 1.6 mm (0.06")
	Max. distance from collecting vessel to analyzer	1 m (3.28 ft)
	Max. height difference from collecting vessel to analyzer	0.5 m (1.64 ft)
	<b>Two channel version</b>	
	<ul style="list-style-type: none"><li>■ Depending on the ordered version, one or two collecting vessels (with or without level measurement) are included in the scope of delivery.</li><li>■ Level measurement is only possible for one channel.</li><li>■ Only one collecting vessel can be mounted at the housing. The second is to be placed nearby the analyzer.</li></ul>	
Sample outlet	Connection	Hose ID 16 mm (0.63")
		– Max. length of closed loop: 1 m (3.28 ft)
		– Open outlet downgrade installed
	Min. volume per measurement	– No combination of several devices to a closed-loop system
		20 ml

## Human Interface

### Display and operating elements

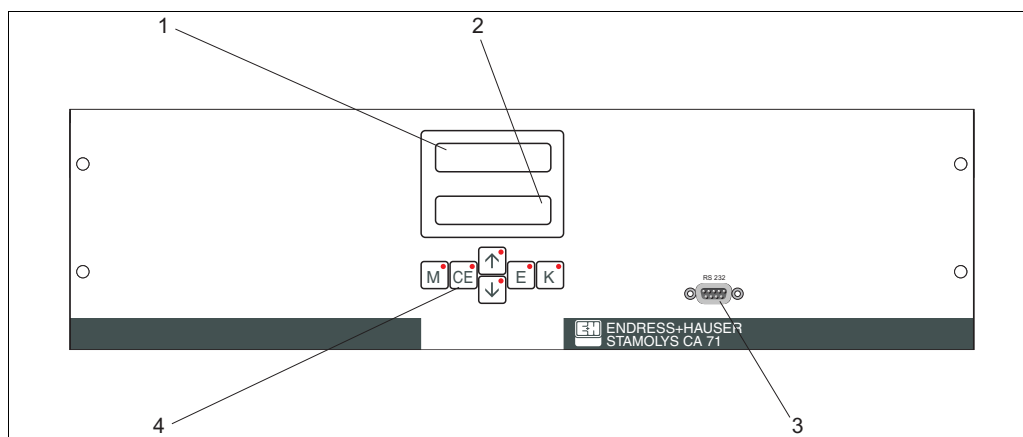

C07-CA71 xxx-19-08-00-xx-005.eps

CA 71 display and operating elements

- 1 LED (measured value)
- 2 LC display (measured value and status)
- 3 Serial interface RS 232
- 4 Operating keys and control LEDs

## Ordering information

### Product structure

Measuring range	
A	Measuring range 0.1 ... 10 mg/l CaCO <sub>3</sub>
B	Measuring range 0.8 ... 80 mg/l CaCO <sub>3</sub>
Y	Special version acc. to customer's specification
Sample transfer	
1	Sample transfer from one measuring point (one-channel version)
2	Sample transfer from two measuring points (two-channel version)
Power supply	
0	Power supply 230 V AC / 50 Hz
1	Power supply 115 V AC / 60 Hz
Collecting vessel for up to 3 analyzers	
A	Without collecting vessel
B	With collecting vessel without level measurement
C	With collecting vessel with level measurement (one-channel version only)
D	With two collecting vessels without level measurement (two-channel version)
Housing version	
1	Without housing
2	With GFK housing
3	With stainless steel 1.4301 (AISI 304) housing
Communication	
A	0/4 ... 20 mA, RS 232
Additional equipment	
1	Quality certificate
2	Quality certificate + set of inactive reagents HA-A
3	Quality certificate + three sets of inactive reagents HA-A
4	Quality certificate + set of inactive reagents HA-B
5	Quality certificate + three sets of inactive reagents HA-B
CA 71 HA -	complete order code

**Scope of delivery**

The scope of delivery comprises:

- an analyzer with mains plug
- a cleaning injector
- a tin of silicone spray
- a Norprene hose, length 2.5 m (8.2 ft), ID 1.6 mm (0.06")
- a Grifflex hose, length 2.0 m (6.56 ft), ID 19 mm (0.75")
- a C-flex hose, length 2.5 m (8.2 ft), ID 3.2 mm (0.12")
- two hose fittings of each size:
  - 1.6 mm x 1.6 mm (0.06" x 0.06")
  - 1.6 mm x 3.2 mm (0.06" x 0.12")
- two T-hose fittings of each size:
  - 1.6 mm x 1.6 mm x 1.6 mm (0.06" x 0.06" x 0.06")
  - 3.2 mm x 3.2 mm x 3.2 mm (0.12" x 0.12" x 0.12")
- an interference suppressor for the current output
- 4 edge covers
- a quality certificate
- Operating Instructions (English).



Note!

Please, order reagents separately with analyzer version CA 71 XX-XXXXXX1.

With all other versions, inactive reagents are included in the scope of delivery. You have to mix the reagents before using them. Please, read the mixing instructions attached to the reagents.

## Certificates and approvals

**CE approval****Declaration of conformity**

The product meets the legal requirements of the harmonised European standards.  
Endress+Hauser confirms compliance with the standards by affixing the **CE** symbol.

**Test reports****Quality certificate**

Depending on the order code, you receive a quality certificate.

With the certificate the manufacturer confirms compliance with all technical regulations and the successful individual testing of your product.

## Accessories

**Reagents and standard solutions**

- ☐ Reagent set, 1 l active reagents HA-A1+HA-A2 each; order no. CAY748-V10AAE
- ☐ Reagent set, 1 l inactive reagents HA-A1+HA-A2 each; order no. CAY748-V10AAH
- ☐ Reagent set, 1 l active reagents HA-B1+HA-B2 each; order no. CAY749-V10AAE
- ☐ Reagent set, 1 l inactive reagents HA-B1+HA-B2 each; order no. CAY749-V10AAH
- ☐ Standard solution 5 mg/l CaCO<sub>3</sub>; order no. CAY750-V10C05AAE
- ☐ Standard solution 10 mg/l CaCO<sub>3</sub>; order no. CAY750-V10C10AAE
- ☐ Standard solution 20 mg/l CaCO<sub>3</sub>; order no. CAY750-V10C20AAE
- ☐ Standard solution 50 mg/l CaCO<sub>3</sub>; order no. CAY750-V10C550AAE
- ☐ Standard solution 180 mg/l CaCO<sub>3</sub>; order no. CAY750-V10C88AAE

**Cleaner for hoses**

- ☐ Cleaning agent, alkaline, 100 ml; order no. CAY746-V01AAE
- ☐ Cleaning agent, acidic, 100 ml; order no. CAY747-V01AAE

**Collecting vessel**

- for sampling from pressurised systems
- results in an unpressurised continuous sample stream
- ☐ Collecting vessel without level measurement; order no. 51512088
- ☐ Collecting vessel with level measurement (conductive); order no. 51512089

## Maintenance kit

- ☐ Maintenance kit CAV 740:
  - 1 set pump hoses yellow/blue
  - 1 set pump hoses black/black
  - 1 set hose connectors per hose setorder no. CAV 740-5C
- ☐ Interference suppressor for control, power and signal lines  
order no. 51512800
- ☐ Silicon spray  
order no. 51504155
- ☐ Valve set, 2 pieces, for two-channel version  
order no. 51512234
- ☐ Upgrade kit for upgrading from one-channel to two-channel version  
order no. 51512640

## Documentation

- ☐ Technical Information Stamoclean CAT430, TI 338C/07/en (order no. 51508729)
- ☐ Technical Information Stamoclean CAT411, TI 349C/07/en (order no. 51508785)
- ☐ Technical Information Stamoclean CAT221, TI 384C/07/en (order no. 51515899)

## International Head Quarters

Endress+Hauser  
GmbH+Co. KG  
Instruments International  
Colmarer Str. 6  
79576 Weil am Rhein  
Deutschland

Tel. +49 76 21 9 75 02  
Fax +49 76 21 9 75 34 5  
[www.endress.com](http://www.endress.com)  
[info@ii.endress.com](mailto:info@ii.endress.com)